Premature Anne

User Guide




American Academy of Pediatrics

DEDICATED TO THE HEALTH OF ALL CHILDREN™


Laerdal


helping save lives

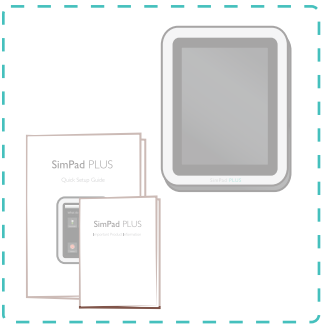



SimPad PLUS
SimPad PLUS


Premature Anne
User Guide
Premature Anne
Premature Anne
Premature Anne

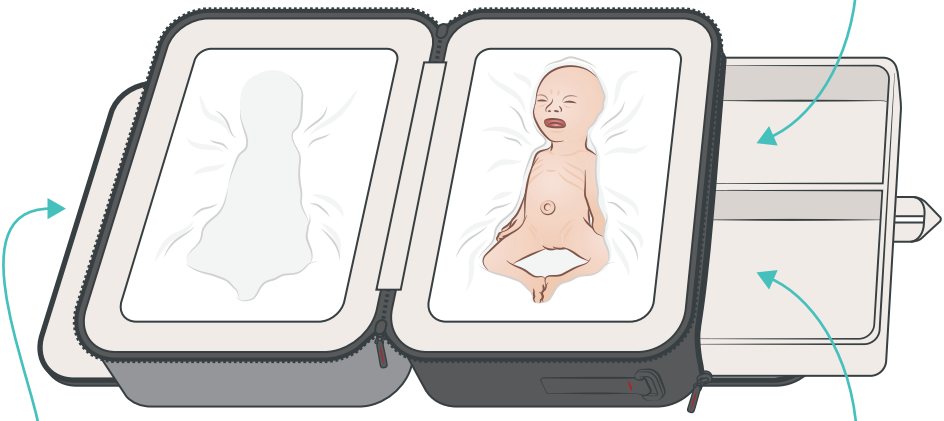

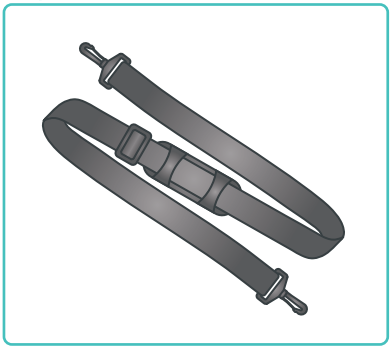

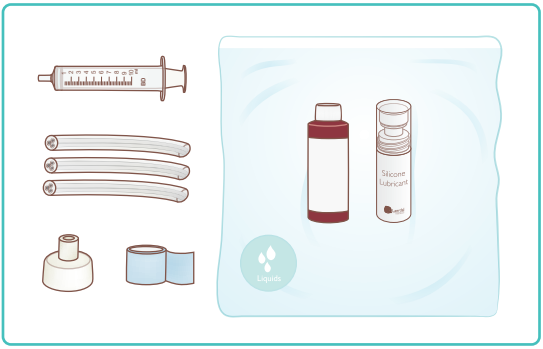
Silicone Lubricant
Liquids

 4

 6

 8

 9

 10

 11

 12


 13


 14


 16


 20


 22

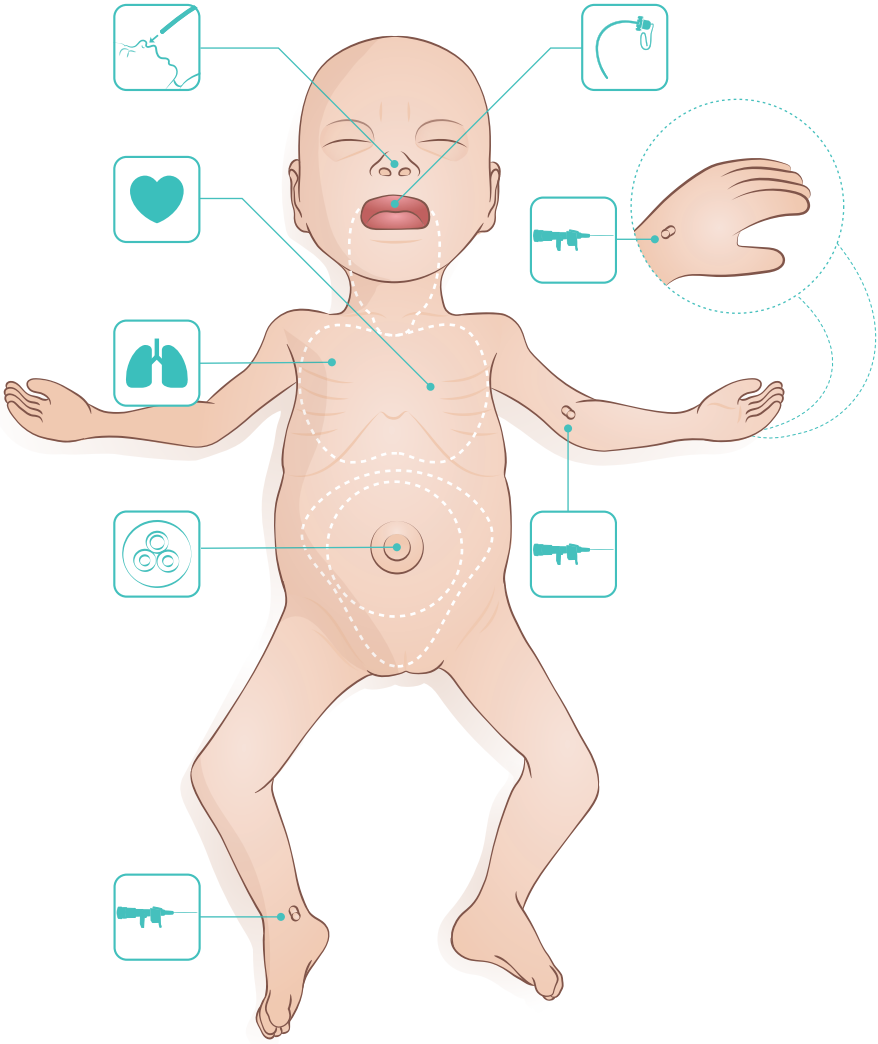


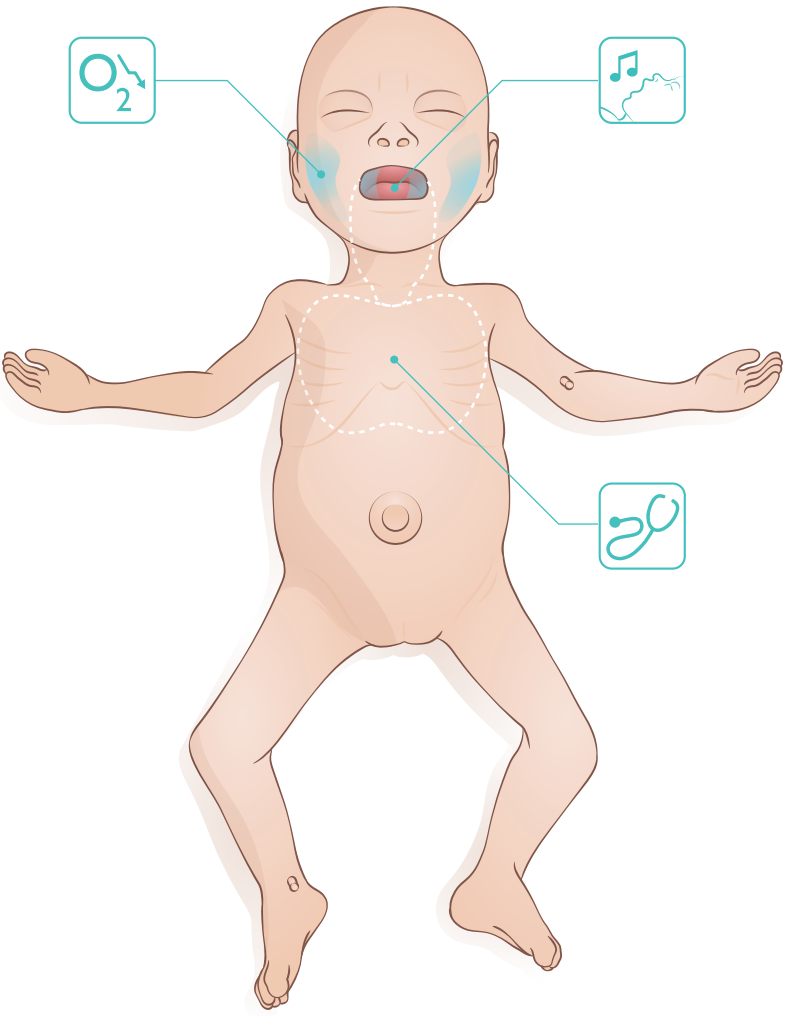


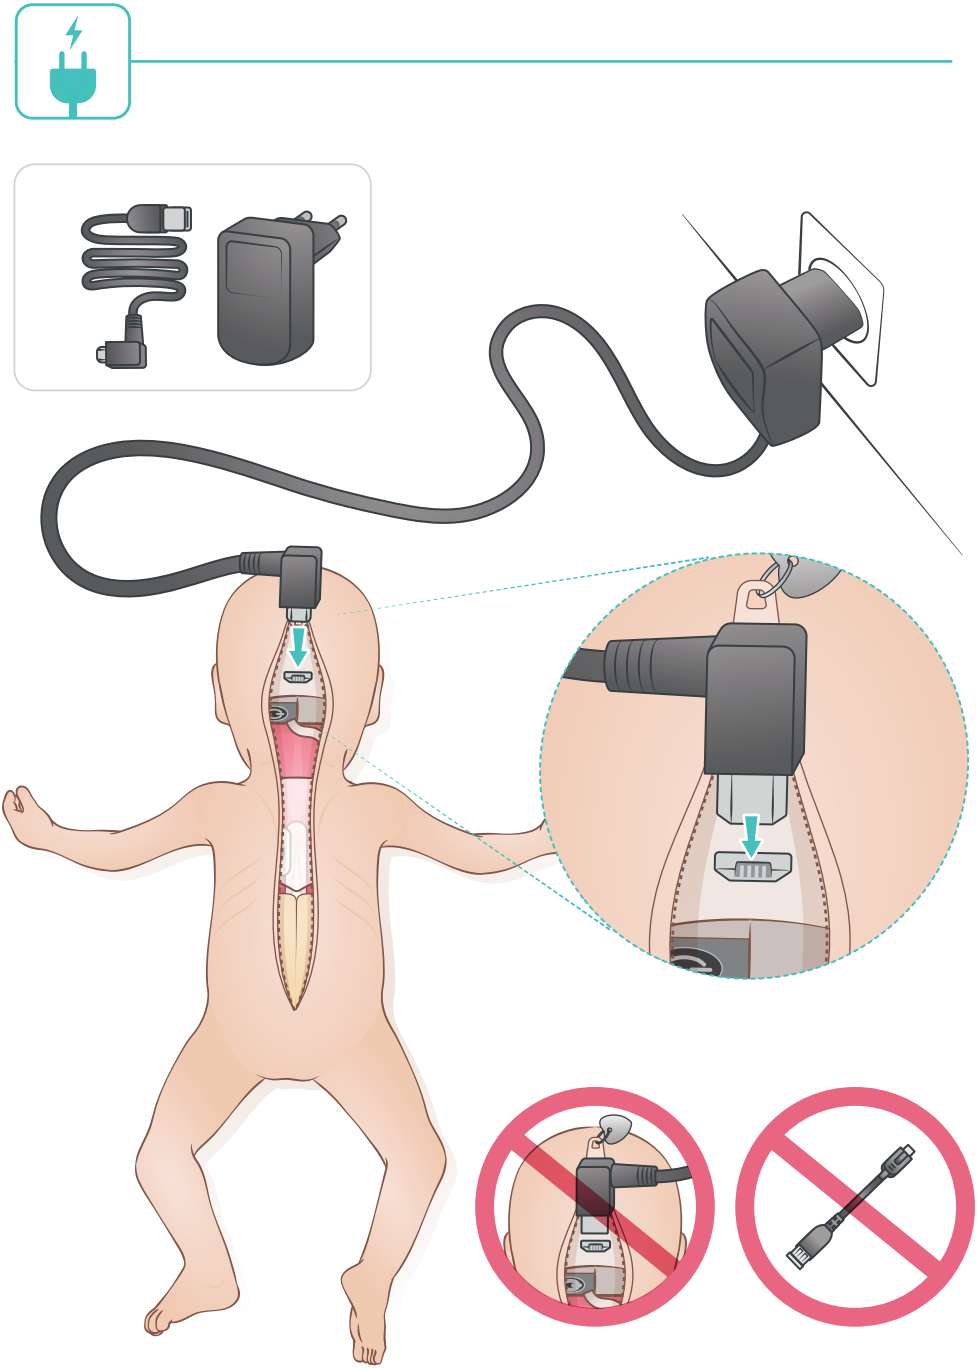


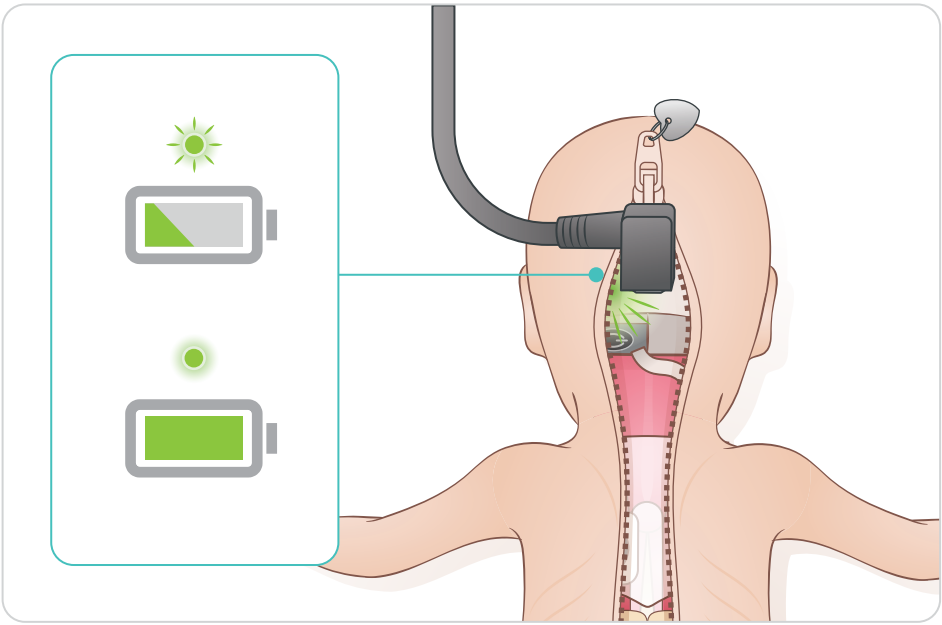

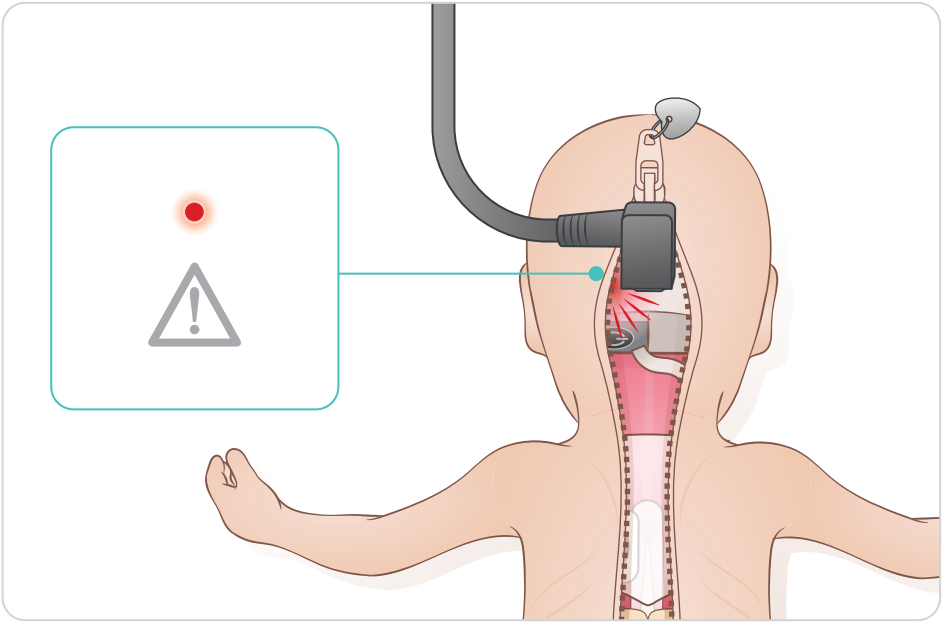

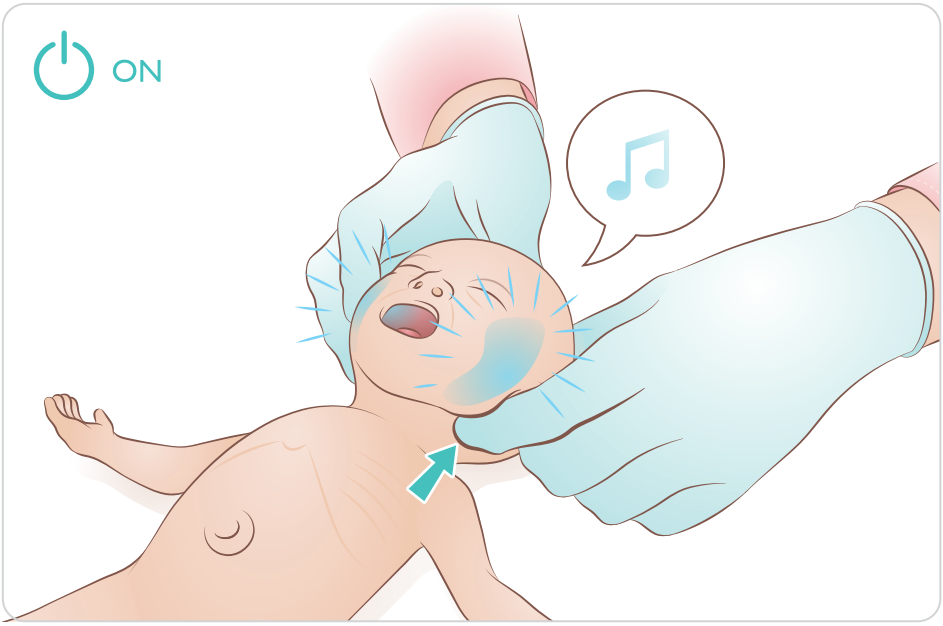

ON

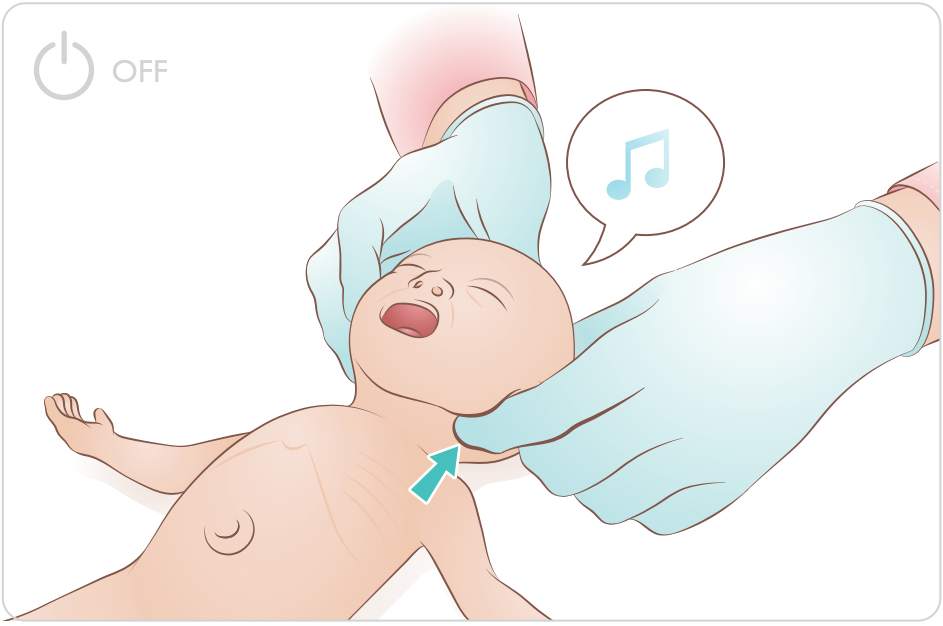

OFF

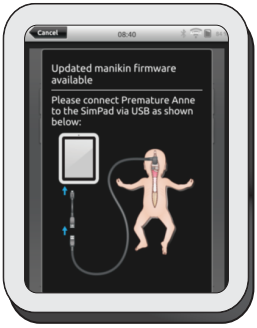

Cancel
08:40
Updated manikin firmware available
Please connect Premature Anne to the SimPad via USB as shown below:





Equipment		Size
	Laryngoscope	Miller 0 / 00
	ET Tube	2.5 mm (oral and nasal)
	Peripheral IV Sites	24 G
	NG/OG tube	6 – 6.5 Fr
	Umbilical Catheter	3.5 Fr Arterial 5 Fr Venous
	Facemask	42 mm

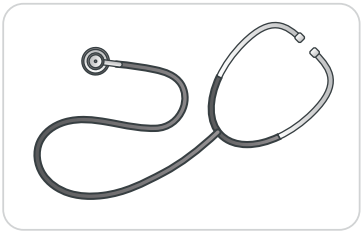

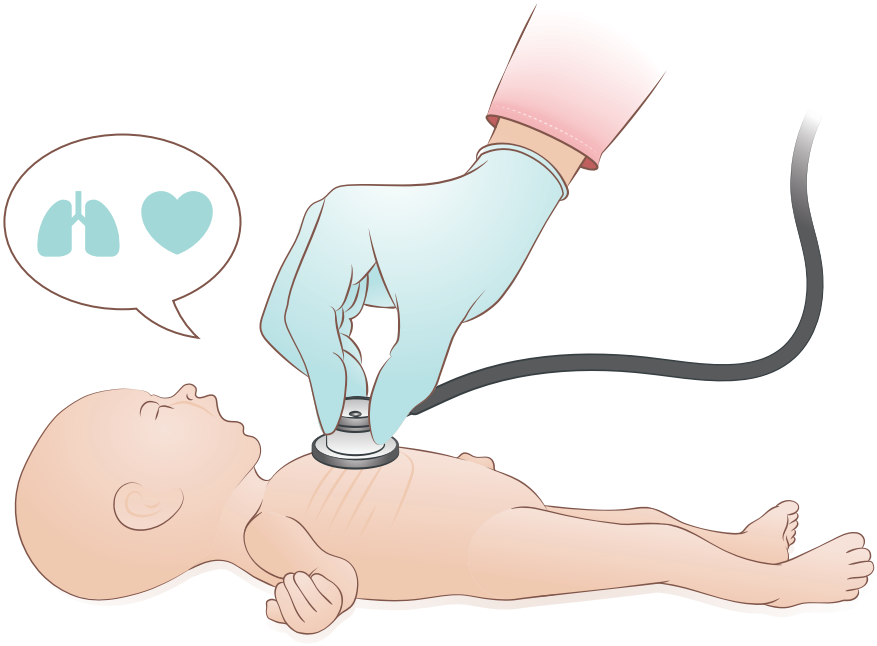

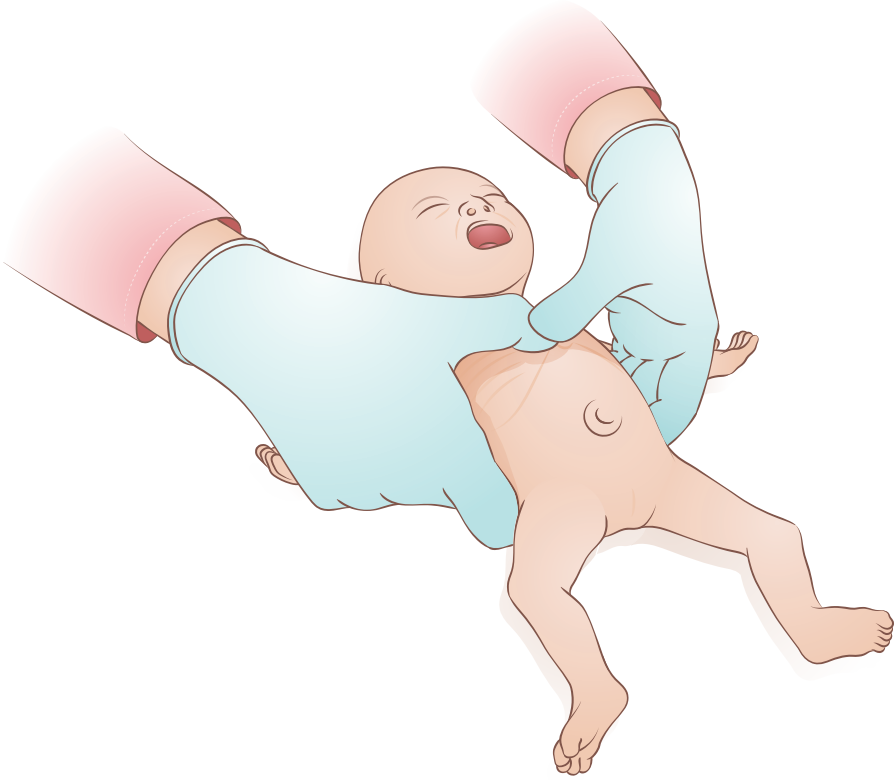


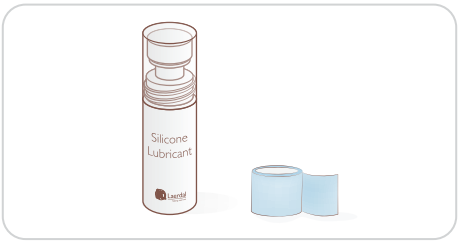

Silicone
Lubricant

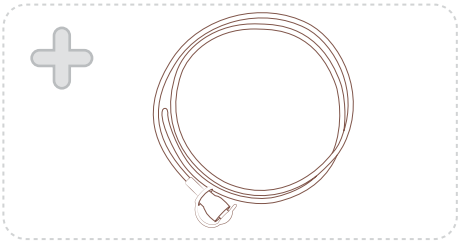




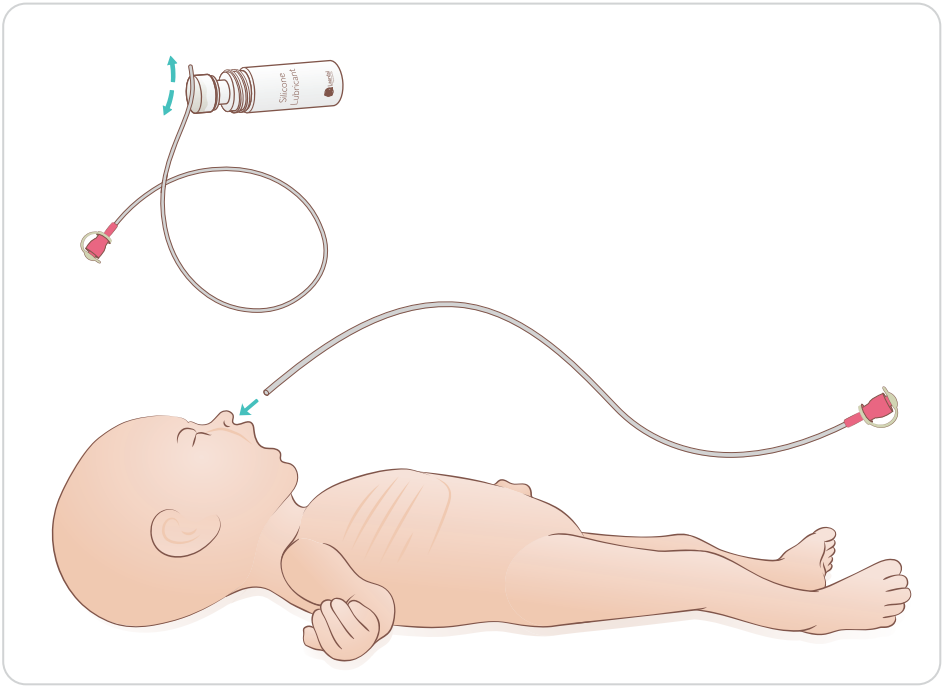



Silicone
Lubricant



Silicone
Lubricant

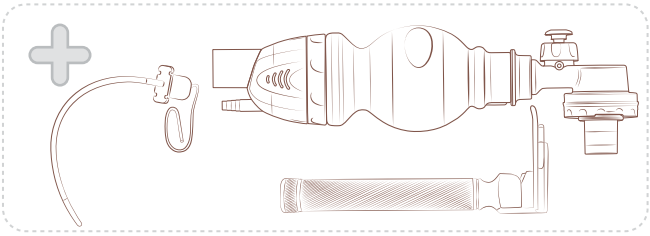








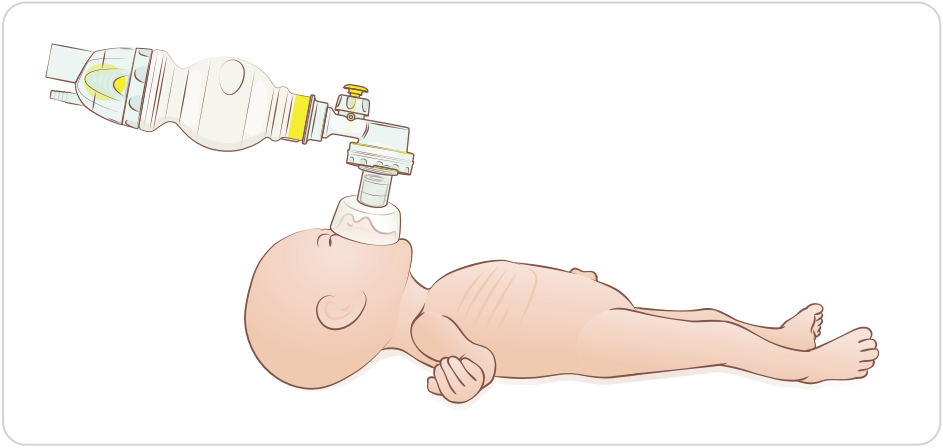


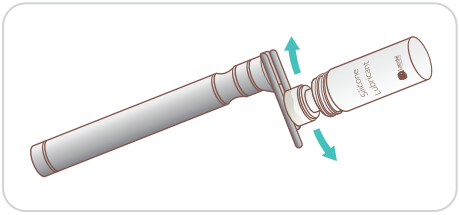

Silicone
Lubricant

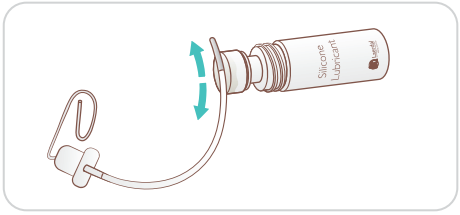

Silicone
Lubricant

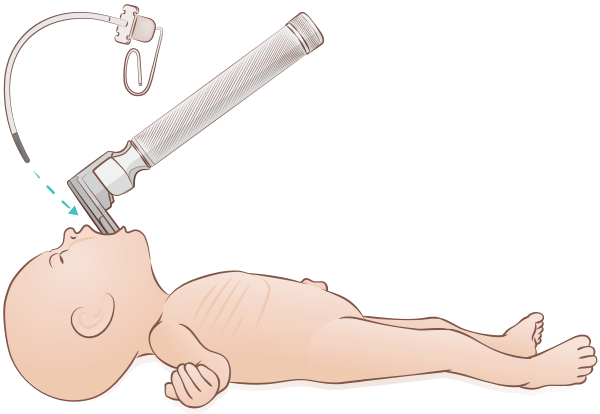


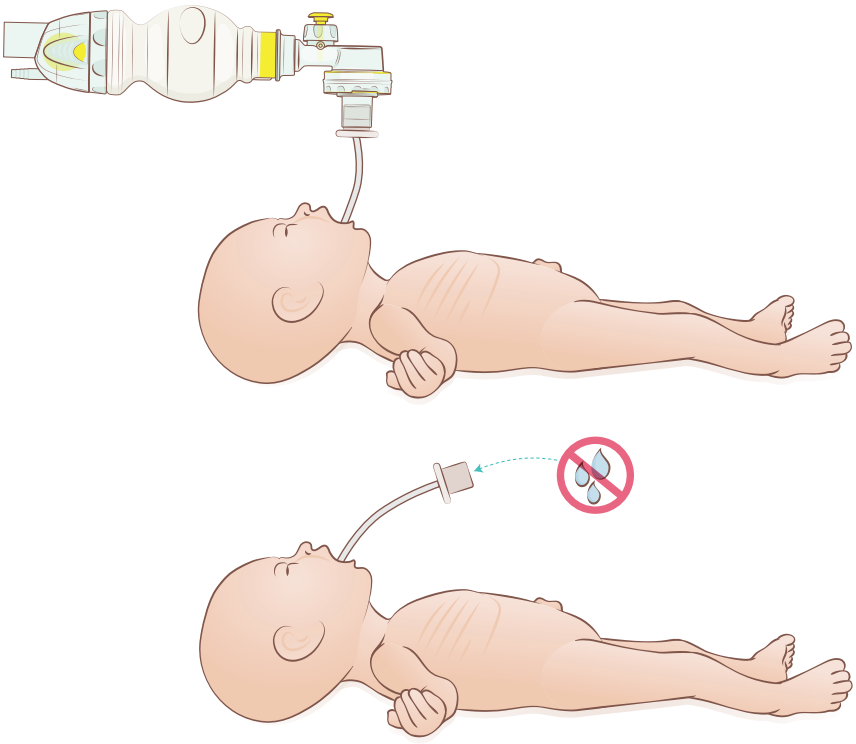


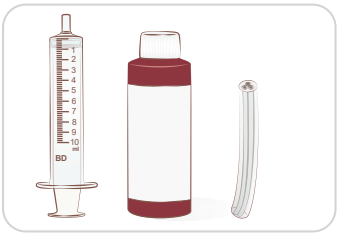


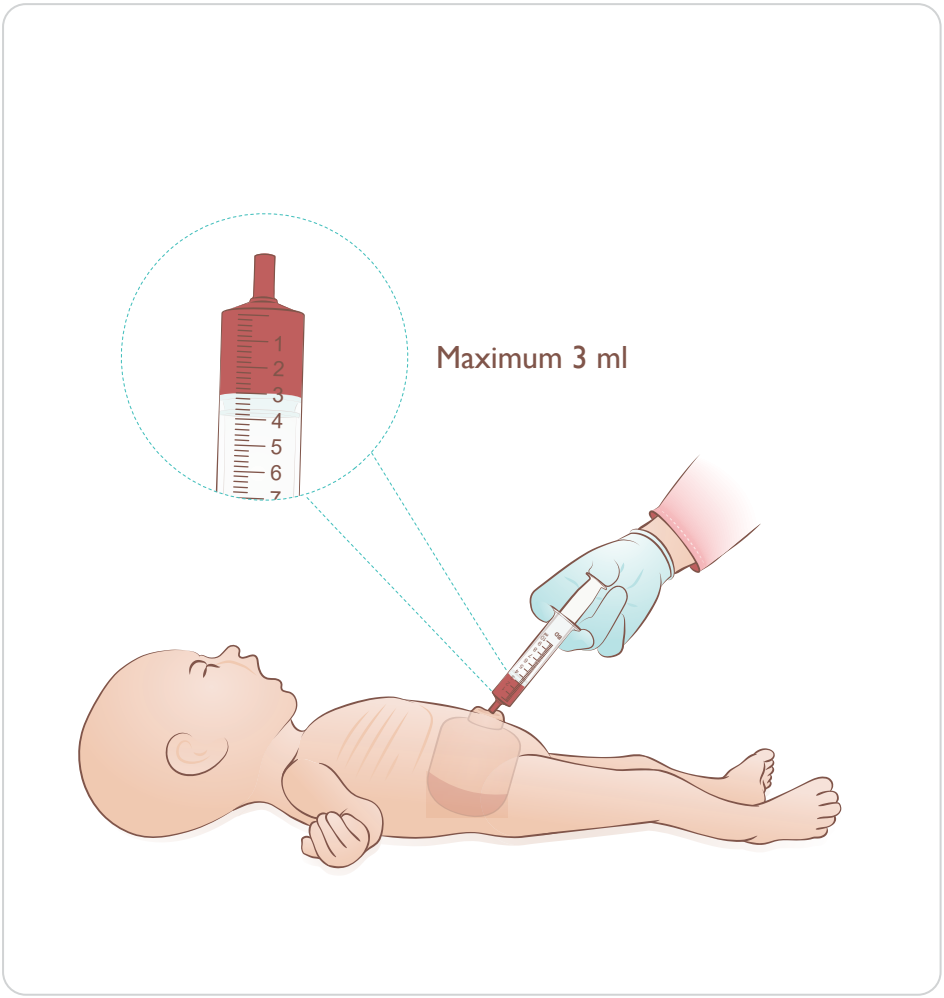

Maximum 3 ml

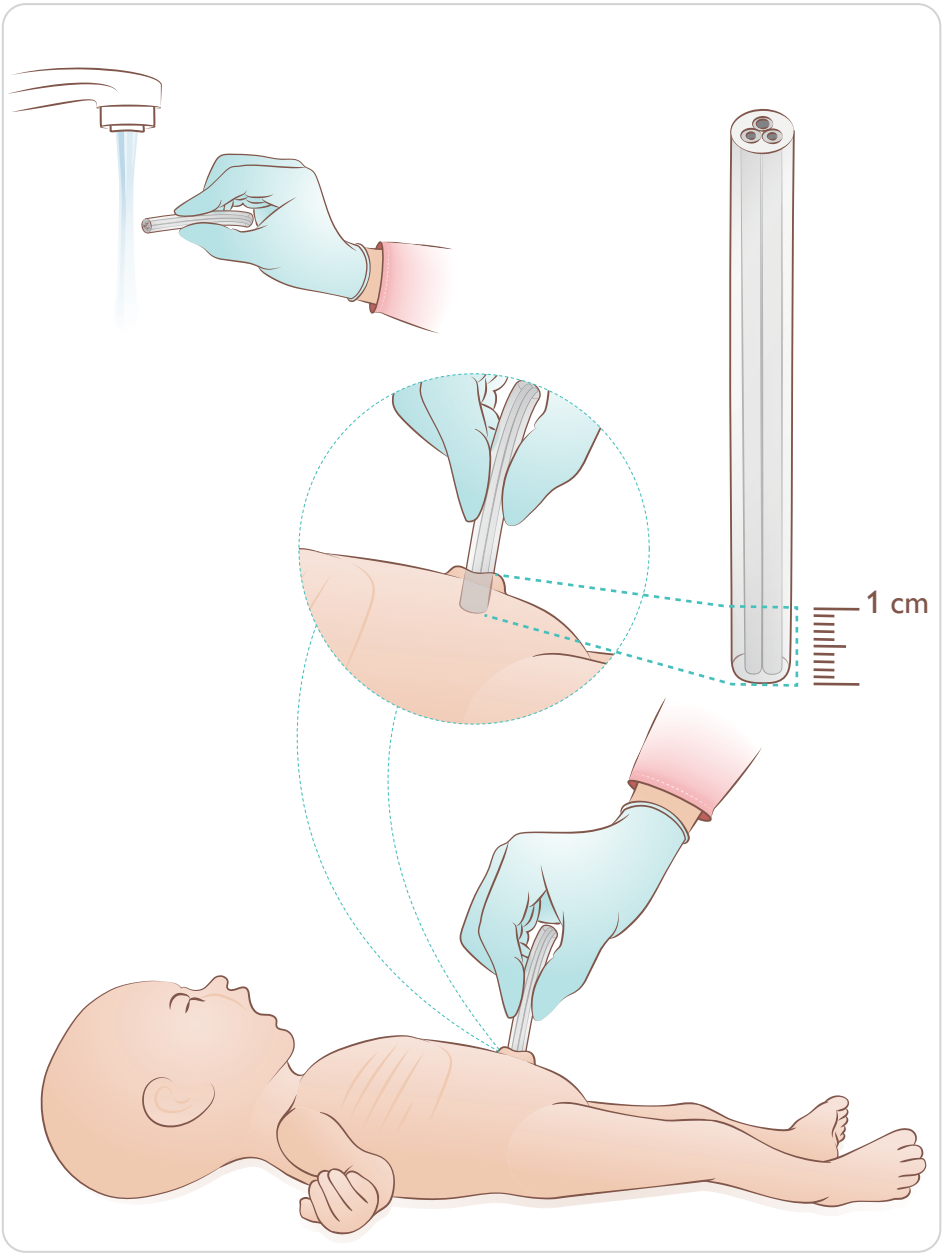

1 cm

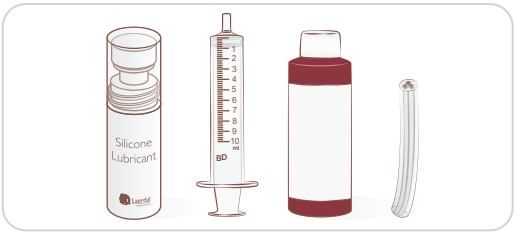

Silicone
Lubricant
BD

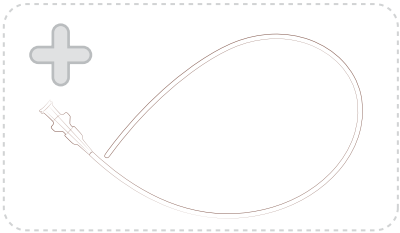


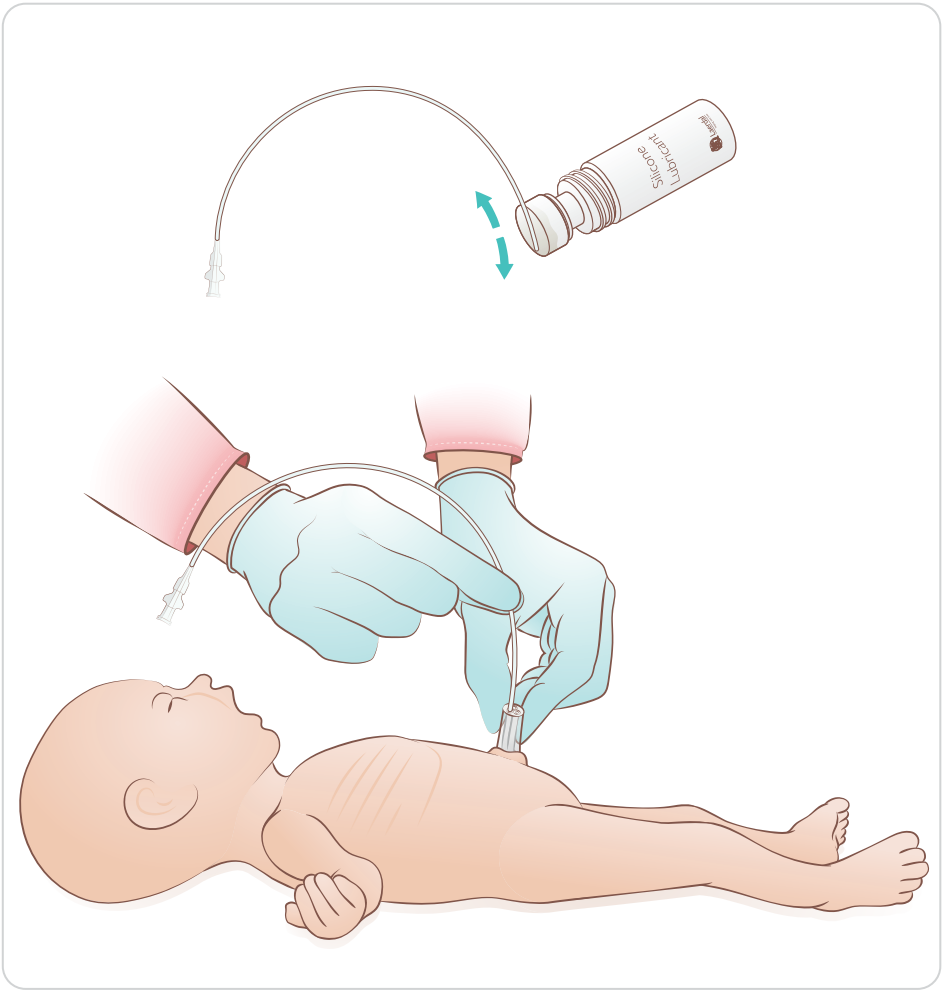
Silicone
Lubricant

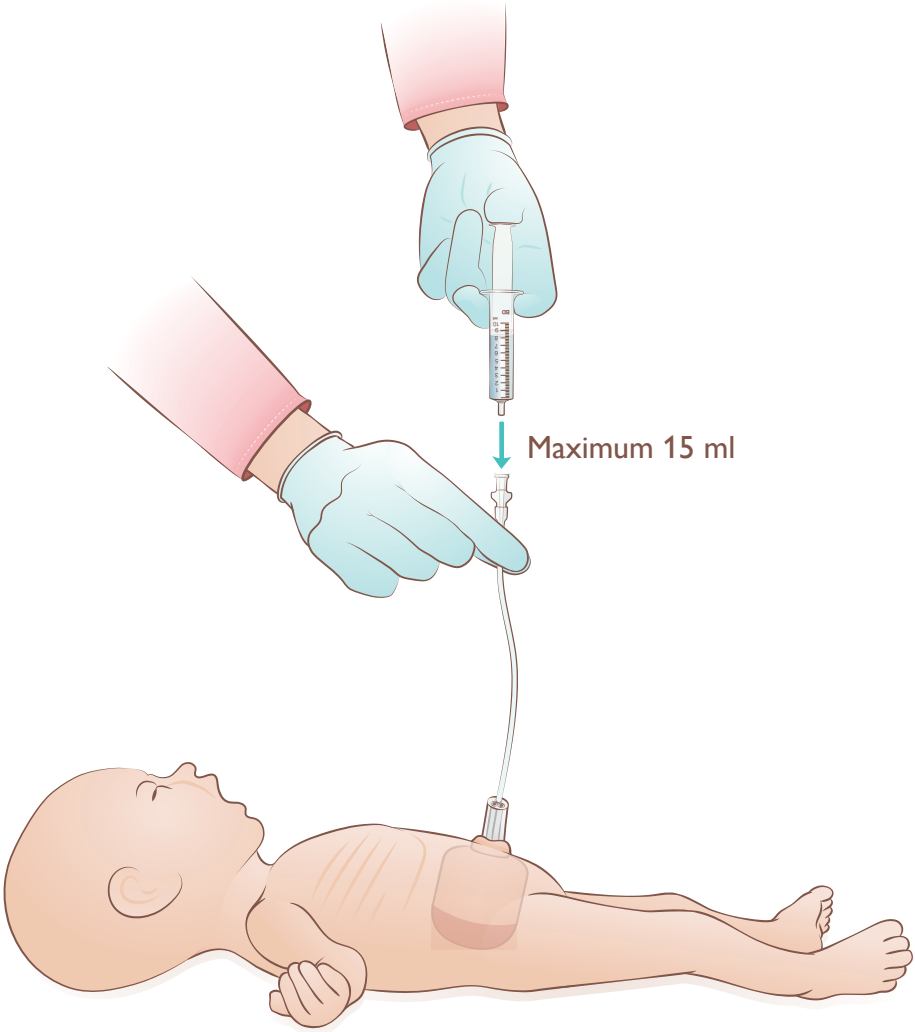

Maximum 15 ml

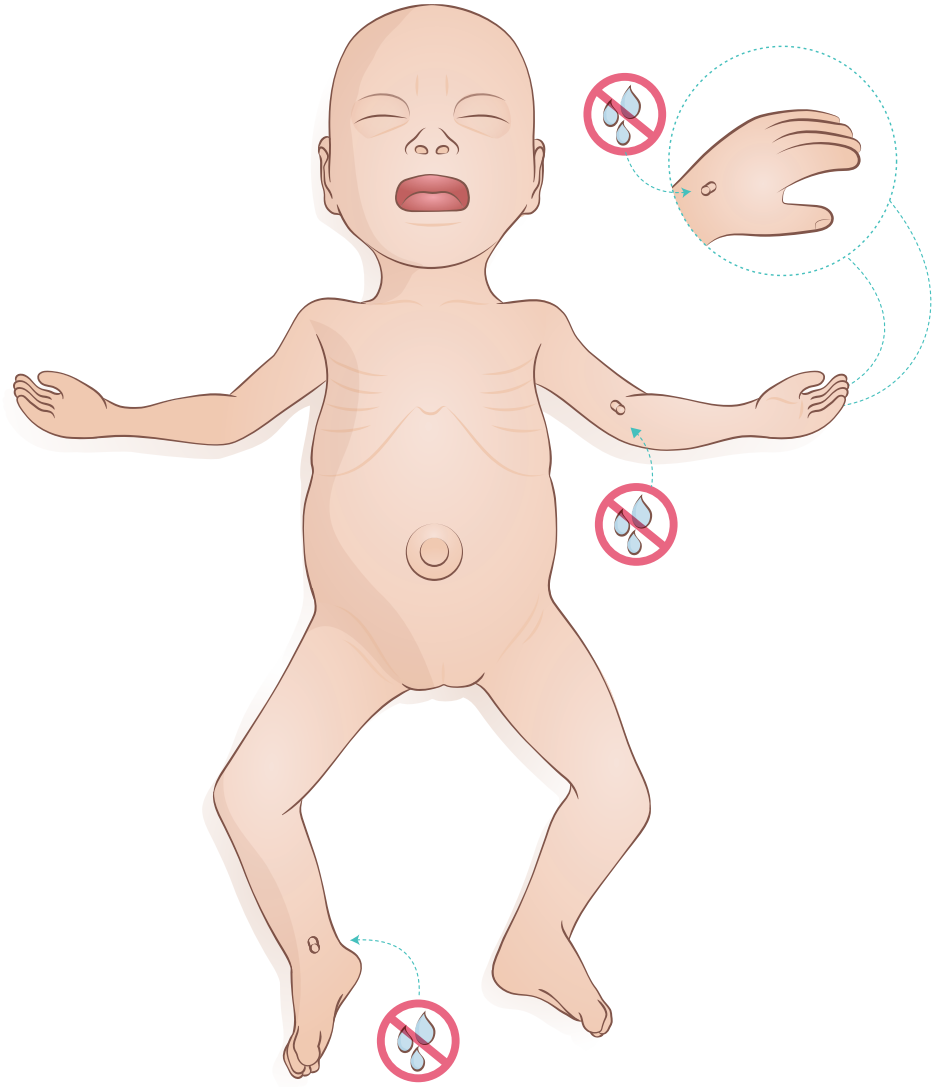

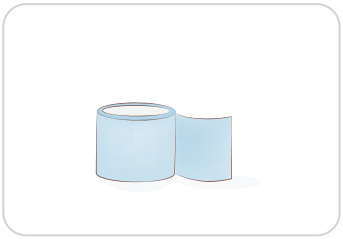


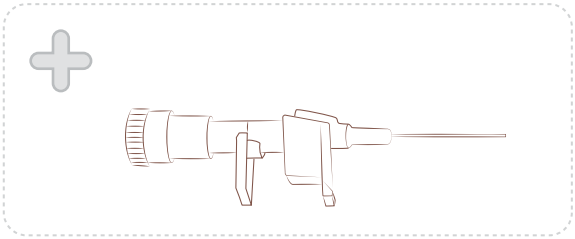

1

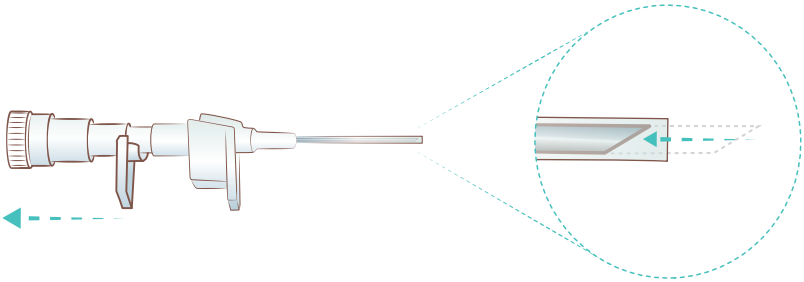


2

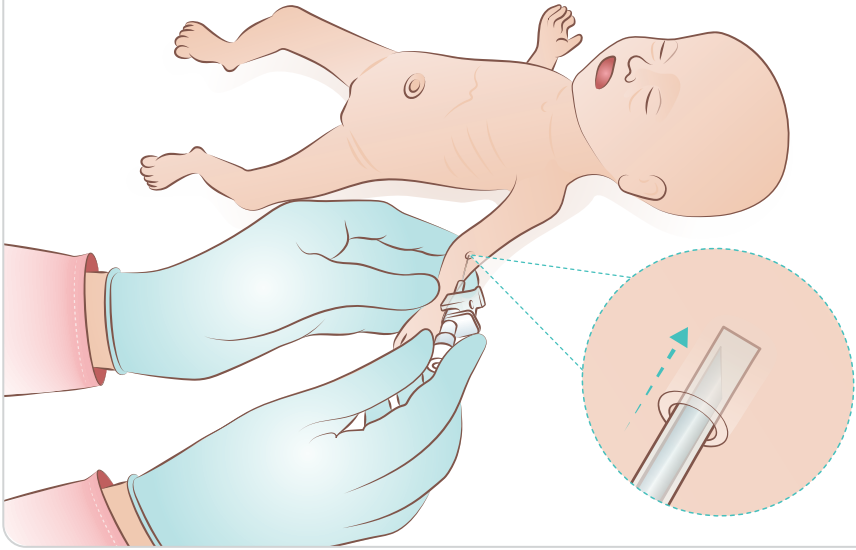






1

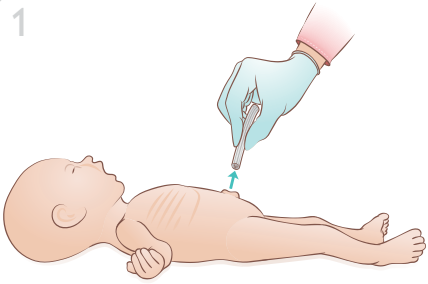



2

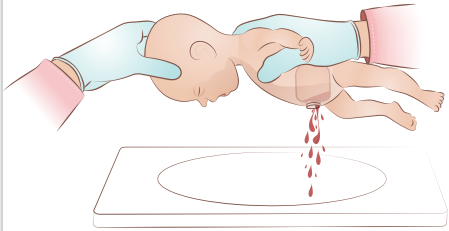

3




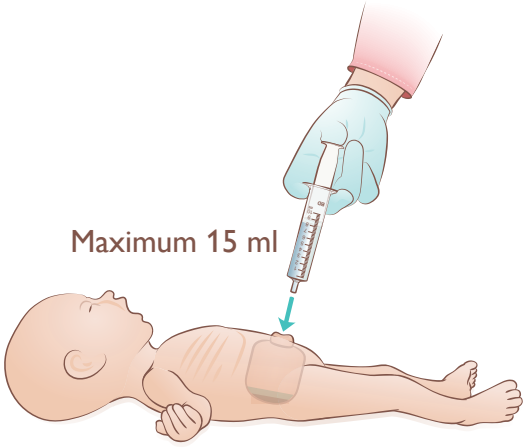

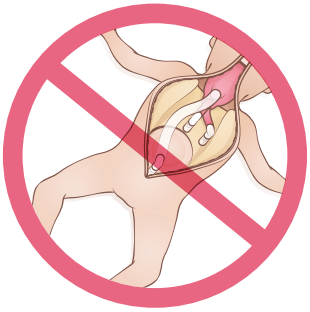



4

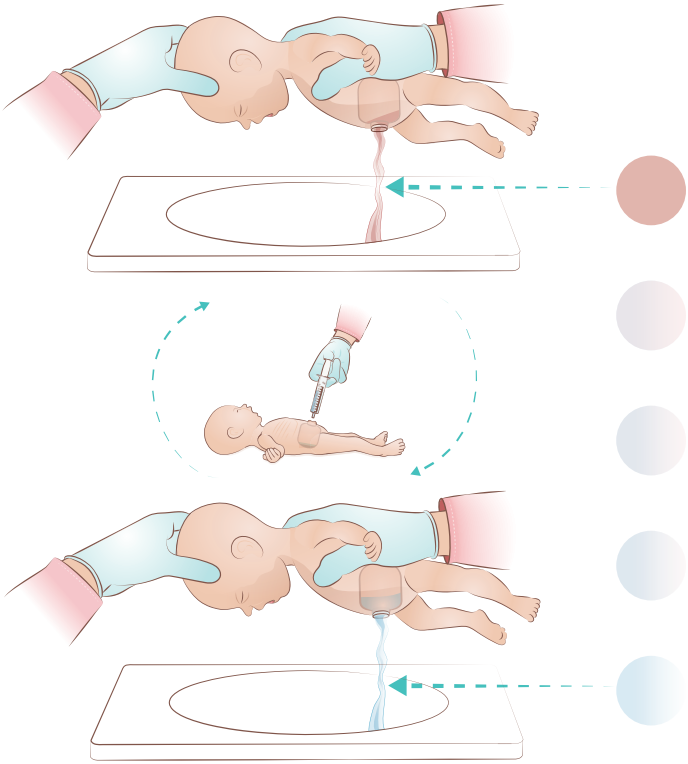







1


2

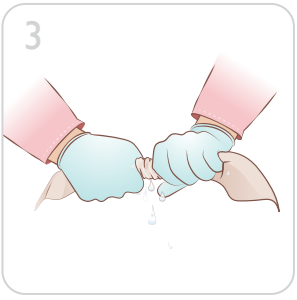
3


4

© 2024 Laerdal Medical AS. All rights reserved.

Laerdal Medical AS
P.O. Box 377
Tanke Svilandsgate 30, 4002 Stavanger, Norway
T: (+47) 51 51 17 00

20-10019 Rev E

American Academy of Pediatrics
DEDICATED TO THE HEALTH OF ALL CHILDREN™

Laerdal
helping save lives